

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
17 November 2005 (17.11.2005)

PCT

(10) International Publication Number
WO 2005/107866 A1

(51) International Patent Classification⁷: A61N 2/00, 5/06

(21) International Application Number:
PCT/EP2005/003304

(22) International Filing Date: 24 March 2005 (24.03.2005)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
2004/0234 11 May 2004 (11.05.2004) BE

(71) Applicant (for all designated States except US): LETEC
NV [BE/BE]; Leuzestraat 91, B-8510 Belleghem (BE).

(72) Inventor; and

(75) Inventor/Applicant (for US only): VANCRAEYENEST,
Marc [BE/BE]; Molstraat 19, B-8870 Izegem (BE).

(74) Agent: OSTYN, Frans; KOB NV, President Kennedypark
31c, B-8500 Kortrijk (BE).


(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:
— with international search report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: SYSTEM FOR INFLUENCING OF A BIOLOGICAL CELLULAR STRUCTURE

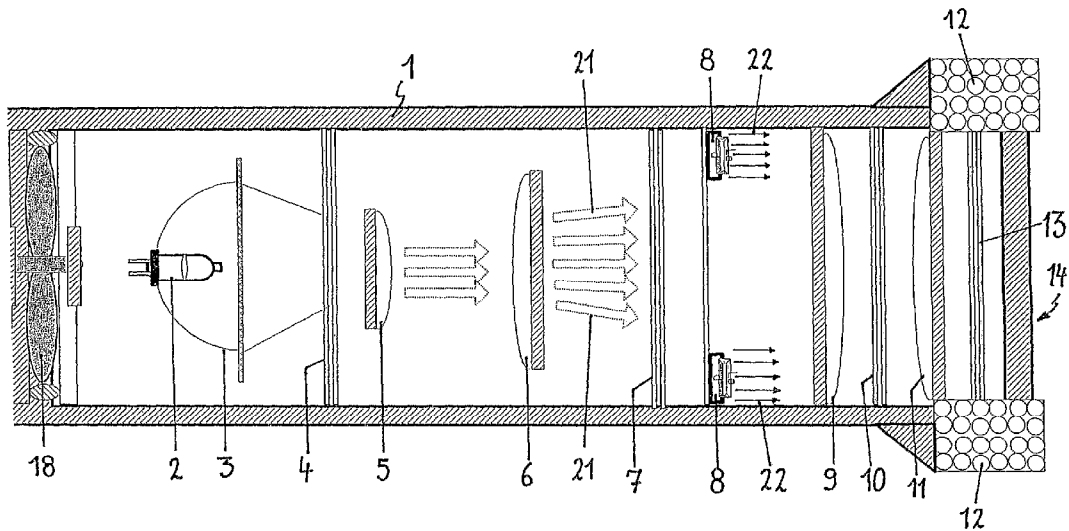

(57) Abstract: This invention relates to a system for influencing of a biological cellular structure, for instance, to generate a therapeutic effect in a human or animal body, making use of a combination of light energy and magnetic energy, said system being provided with at least one light source (2), (8), a magnetic energy source (12), which is preferably capable of generating a pulsing magnetic field, and devices to adjust and/or modulate the frequencies and/or phases and/or amplitudes of the light and/or the magnetic field so that resonances and/or interferences may be obtained in the biological cellular structure. The system preferably comprises a first (2) and a second light source (8), which generate light with a different coherence, in which the light coming from the first light source (2) and the light coming from the second light source (8) is preferably used alternately and/or with a phase shift and is polarized.

WO 2005/107866 A1

System for influencing of a biological cellular structure

5 This invention relates to a system for influencing a biological cellular structure, in which use is made of a combination of light energy and magnetic energy.

This invention relates in particular to a system for realising beneficial effects on a biological cellular structure in a human, an animal or a plant. More in particular, it
10 relates to a system for realizing specific therapeutic effects in humans and animals.

It has long been known that light of certain frequencies can create certain therapeutic effects on a living creature. Applications thereof are generally indicated by the term light therapy. There are instruments for application of light therapy that comprise a
15 so-called coherent light source, such as a laser system. These systems have the disadvantage that their use can be hazardous. Other well-known instruments comprise a source of incoherent light, such as a full-spectrum lamp.

Besides these, also the magnetic field therapy is known, in which magnetic energy is
20 used to obtain a beneficial influence on the health of the human.

In addition, instruments that combine the effects of light therapy and magnetic energy have already been developed. Such device is described in a number of patent publications, as for instance in French patent application No. 2 639 834. In this
25 document, an instrument is described by which pain, inflammation and local energy disturbances can be treated. With this instrument, light of a certain spectrum as well as a magnetic or an electric field can be realised. This instrument allows orienting the so-realised electrical and magnetic fields in relation to the treated tissue. This kind of instruments has only a very limited number of fields of application and they are
30 furthermore not very effective.

In European patent publication EP 0 228 537 A2 and in German patent publication DE 3 101 715 A1, instruments are described with which we can combine light therapy with a treatment with magnetic energy. In such treatment, we obtain at the most a combination of the known effects of infrared light therapy and the known effects of the magnetic field therapy.

In addition, the presently known instruments have the disadvantage that the light energy cannot penetrate deep enough (at the most a few mm) in the tissue, so that the efficiency of these instruments leaves much to be desired. Their therapeutic effect is rather minimal and within a very limited field of application. Their field of application is most often limited to tissue heating and pain relief.

The object of this invention is to realise a system by which, when influencing a biological cellular structure, greater efficiency is obtained through a combination of light energy and magnetic energy and this within a very broad field of application,

This objective is obtained because this system, besides having at least one light source and a magnetic energy source, also comprises devices to adjust and/or modulate the frequencies and/or the phases and/or the amplitudes of the light and/or the magnetic field so that resonances and/or interferences may be obtained in the biological cellular structure.

The magnetic energy also ensures that the light energy penetrates deeper into the tissue and reaches certain cells that with the presently known instruments were not reached or were insufficiently reached.

The effects of electromagnetic fields on a living organism can be explained as follows. Each living organism is an electromagnetic field that, precisely because of its physical properties, is a living creature. All parts of, for instance, a human body, i.e. its very many billion [UK milliard] cells, are built from complex compounds that themselves consist of molecules. Each molecule has its atoms and each atom has its

own little electromagnetic field. This so-called little magnet is kept in existence by positively charged protons and there-around rotating negatively charged electrons.

5 Hormones, vitamins, (trace) elements, lipids, amino acids, carbohydrates, salts, bases, acids, but also water, oxygen, carbonic acid gas and nitrogen have, by their molecular composition, a proper chemical identity from the periodic system of elements. In addition, they have a specific electromagnetic field or charge, which is built up and composed by the corresponding atoms. One could state that the sum of the electrical charge of each atom in a molecule gives such molecule a specific
10 vibration. We call this the specific vibration frequency or resonance frequency. Consequently, cells, tissues and organs also have electromagnetic properties.

Besides its built-in reinforcement structures, the cell wall also has specific filtration functions. Only very special molecules are assisted inwardly or outwardly, so that the
15 quality of the inside of the cell, the cytoplasm, is preserved and a certain pressure and cell shape is maintained. For instance, a reaction between a hormone and a cell receptor is determined by the fact that both have a mutually compatible vibration. If one of the vibrations weakens, the reaction will take place only partially.

20 To put it simply, the voltages (potentials) at the inside and outside of the cell wall form the motor of the transport mechanisms through the cell wall of, for instance, ions, food, waste products and cell products. In addition, growth, cell division and cell movement processes can only take place if the correct transport means and membrane potential are present. Magnetic fields influence this potential. In a similar
25 manner, also smaller units such as tissues, cells and cell organelles may obtain 'misinformation' in case of turning magnetic fields or alternating magnetic fields. Precisely what tissue and what process will be influenced depends on factors such as the type of magnetic field and the frequency of its alternations.

30 In a conductive structure, each change in the electromagnetic field will induce a small electric current, and a voltage difference will be created between the

extremities of such structure. In other words, the structure becomes polarized. Some parts within the structure can then also become polarized. The larger or the longer the structure, the larger the voltage difference can become. Basically, elongated structures will operate very well as an antenna for the electromagnetic fields. Hence,
5 basically, structures such as long nerve ends, gliascheden, liquid cavities in the brain and spinal cord and lymph and blood vessels can serve as 'receivers'.

Most living organisms also have a kind of detector for magnetic fields, namely iron-containing ferritin that is especially useful for our orientation.

10

We often see from experiments that we can only produce the studied effects when the frequency lies within a rather narrow window. Furthermore, such influencing may have either a stimulating or a limiting effect. It is exactly this kind of influencing that we look for with the system in accordance with this invention.

15

By creating resonances and/or interferences in specific cells, we can influence biological cellular structures in order to obtain a specific therapeutic effect.

20

Natural oscillations can be observed in a vast range of organisms and tissues, and at very different frequencies, such as protein molecules and protein structures in animal cell walls (millions of Hertz), cell walls with their contractile protein filaments (a few thousand Hertz), some neurones that operate as 'biological clock' (a few Hertz).

25

The system in accordance with this invention preferably comprises two different light sources, called a first and a second light source, whilst the second light source is capable of generating light that is essentially more coherent than the light from the first light source.

30

Such system has the advantage that it works even more efficiently within a yet broader field of application. Indeed, when the system is applied to cellular structures of a human or an animal, we observe that, by using two light sources with different

coherence, both the received stimuli (by one light source) and the response from the brain (by the other light source) are reinforced according to the well-known principle of the complex-reflex method.

- 5 Said first light source can for instance be a full-spectrum lamp. The second light source can for instance be a LED light source that generates mainly coherent light.

In a very preferred configuration, the system comprises devices to use alternately and/or with a phase shift light from the first light source and light from the second
10 light source. This enables triggering specific actions (reflex actions of the neurotransmitters) on specific cells (photoreceptors and cyton cells) and tissues, in which certain biochemical processes are strongly influenced, such as acid-base management and the Ca^{++} channels. Influencing the acid-base management may have an analgesic effect that for instance may produce some pain relief through the stimuli
15 of the endorphins in the skin.

In addition, by photon penetration and modulation, the immune response will be reinforced both at biological cellular and hormonal level, so that, through a correction of the hormonal (endocrine) and emotional imbalance, the body's defence
20 mechanism can react optimally to symptoms of stress, pressure and fatigue.

We obtain a very efficient system if it also is capable of generating pulsing magnetic fields.

- 25 By this, by means of specific weak electromagnetic fields, we can perform a bio-stimulation at skin level, by which cell regeneration is strongly stimulated and the tissues, for instance absorb more oxygen. This may stimulate the healing of wounds by, for instance, stimuli of the infiltrations of neutrophils, macrophages, and the formation of Scavenger cells that in turn take care of the evacuation of infectious
30 micro-organisms.

The whole rearranges the disturbed electrical poles of the cell membrane (positively and negatively charged particles), by which the enzymes and their receptors form stimuli for the metabolism and for the creation of energy reserves at cellular level by influencing the mitochondria and stimuli of the ATP, which in turn feeds the cellular
5 chemical processes, in particular by modification of the cellular membrane potential.

The system becomes even more efficient and especially easy to use within its very broad field of application if it also comprises devices to have the frequencies of the magnetic field pulses and/or the light source pulses vary automatically in accordance
10 with a predetermined pattern and/or within a predetermined range, so as to obtain said resonances and/or interferences.

In another preferred configuration, the system also comprises devices to polarize the light coming from the first light source and/or the light coming from the second light
15 source.

By such polarisation, one component (the electrical component of the electromagnetic component) of the light is eliminated. By this organising effect of the polarisation, we succeed in influencing biochemical processes through the skin
20 nerves, in which especially mechanoreceptors, neuroreceptors, thermal receptors, chemical receptors, light receptors or the acid-base changes are influenced or the Ca^{++} channels and neurotransmitters are stimulated.

The second light source comprises preferably one or several LED light sources that
25 are capable of generating single-phase light.

The system in accordance with this invention is preferably configured to generate a therapeutic effect in a human or animal body.

30 To further explain the technical properties and operation of this invention and to indicate additional advantages and peculiarities of it, a more detailed description of

an instrument in accordance with this invention follows below. However, we insist on the fact that nothing in the description hereunder may be interpreted as a limitation of the claimed patent rights or of the field of application of the system in accordance with this invention.

5

In this detailed description, reference is made to the enclosed drawings by means of numbers. These drawings are:

- 10 • figures 1a and 1b, which show a schematic cross-section of the casing with light sources and magnetic energy source for two different configurations of an instrument in accordance with this invention;
- figure 2, which illustrates by a block diagram the operating principle of the instrument in accordance with the invention;
- 15 • figure 3, which shows by a block diagram the different components of the electronic part of the instrument in accordance with the invention; and
- figure 4, which presents by a block diagram the oscillator modules and the
20 trigger generators of the instrument in accordance with the invention.

In a first specific configuration (see figure 1a), the instrument in accordance with this invention comprises an elongated casing (1) with a open side (14). In this casing (1), a broad-spectrum lamp (2) with reflector (3) is provided. Between this lamp (2), a
25 source of incoherent light, and the open side (14) of the casing (1) we find in succession in the casing (1): an infrared filter (4), a first (5) and a second lens (6), a spectrum filter and/or colour filter (7), a series of LEDs arranged in a ring (8), a third lens (9), a polarisation filter (10), a fourth lens (11), an electromagnetic coil (12) and a protective lens (13) with optimised diaphragm.

30

A second specific configuration (see figure 1b) differs from the first one in that the broad-spectrum lamp (2) is provided with a closed reflector (15) with lens (15a), and in that between the infrared filter (4) and the spectrum filter (7), the first (5) and second lens (6) are replaced by an integrator (16) and one single lens (17). The closed reflector (15) serves to bring the light bundled and with the desired width forward, through reflection on the aluminium sheath, so that we obtain maximum efficiency on the surface that we wish to illuminate.

The broad-spectrum lamp (2) is in both configurations capable of generating a power density of at least 15 mW/cm and a light energy with a value of at least 4 Joule per minute and per cm.

The working of the instrument can be further illustrated by means of figures 1a, 1b and 2. The broad-spectrum lamp (2) delivers incoherent light (20) that is filtered in the infrared filter (4) and bundled by the first (5) and the second lens (6) (in the configuration in accordance with figure 1a) or by the integrator (16) and lens (17) (in the configuration in accordance with figure 1b), so that a bundle of homogenous light (21) is obtained, which is mixed with the coherent light (22) coming from the LEDs (8) by means of the pair of lenses (9), (11). This light is polarised by the polarisation filter (10).

The light coming from the broad spectrum-lamp (2) and the light coming from the LEDs (8) is preferably used alternately. Polarisation preferably takes place with a Brewster polariser or a light transmission system. The light leaves the casing (1) via a protective lens (13) with optimised diaphragm, which ensures that the exiting light bundle can cover a specific surface, in which stray light is eliminated to the maximum possible extent by cutting. The inside of the casing (1) is cooled by means of a fan (18) installed behind the lamp (2).

At the same time, a pulsing magnetic field (23) is generated by means of the electromagnetic coil (12). This magnetic field (23) is used together with the light

energy so that the light waves operate as a carrying wave for the magnetic pulses. This is finally the actual end product (26) that leaves the casing and which is used to influence a biological cellular structure.

5 Meanwhile, the light sources (2), (8) and the electromagnetic coil (12) are controlled by a control system (drive) (24), in order to adjust its frequencies and/or phases and/or amplitudes, so that resonances and/or interferences may be obtained in a treatable biological cellular structure. In figure 2, modulation is represented by block (25).

10

This control system (24) fulfils in particular the following functions in the instrument: pulse wave modulation, dimming and triggering and control of the oscillators (39) and the cooling fan (18).

15 For this, the control system (24) comprises a microcomputer system with the following components (see figure 3). An input module (30) and a screen module (31) for the user, a PC interface module (32), namely RS 232 or USB, a card reading module (33), a sound module (34), an oscillator module (35), drive circuits/dimmer circuits (36), a power supply (37) and an MC microcontroller (38).

20

The oscillator module (35) comprises (see figure 4) a series of oscillators (39) that are capable of generating square or saw-tooth pulses, by which, through a number of pulse width modulators (41) and trigger generators (42) the LEDs (8) and the electromagnetic coil (12) are driven. The trigger generators (42) co-ordinate the control of the different light sources (2), (8). Figure 4 also shows the power supply (43) and next to it the pulse width modulator (41) of the drive circuits/dimmer circuits (36).

25

The microprocessor modules control both the broad-spectrum light source (2) and the LEDs (8). To fulfil its function properly, the microcomputer has at least a bus system, a memory, a timer/counter, a number of input/output channels, a PC

30

interface bus, a control system and a program that coordinates and monitors the whole.

5 The electronic part can be programmed to automatically generate and run through a pattern of specific frequencies and thus, by means of precision settings, generate resonances in the cellular structure of tissues and bio-cellular matrix, in general in a biological cellular structure.

10 The two different light sources can be driven separately and combined in accordance with a specific modulation pattern and this synchronously with the employed magnetic fields, this in order to modify for instance the reflection and absorption behaviour of the treated tissue at a specifically to be set resonance frequency, by which very deep tissue penetration can be obtained. An additional modulation takes care of the cellular information transfer.

15 To mix the light of the first and the second light source, the instrument can be provided with an integrator pipe or a fibre optic channel (not shown in figures 1a and 1b). When a fibre optic channel is used, we obtain a very pronounced flank cut in the UV and infrared light frequency ranges. By this, any heating of the treated biological cellular structure is prevented. Of course, this enhances the safety and the user
20 friendliness of the instrument.

To obtain an efficiently working instrument, it is important that the emitted light is homogenous over a relatively large surface, this in order to reach at once the largest
25 possible surface of the to be treated cellular structure. By use of the first (5) and the second lens (6) in the instrument in accordance with figure 1b, we ensure that this surface is sufficiently large. The lens (5) is used to draw the central homogenous part of the light out of the light bundle. Then, by means of another lens (6), this homogenous part is enhanced to a light bundle that is homogenous over a relatively
30 large surface.

For instance, to be able to work efficiently in case of wound treatment, we will ensure that the light is homogenous on an a surface of at least 100 cm². For other applications for instance, it will be indicated to have a homogenous light on a surface that corresponds with the size of the head or of another body part of a person or
5 animal.

The instrument in accordance with this invention can be used in a large variety of fields of application, such as obtaining beneficial therapeutic effects for arthritis/arthrosis. In this case, the instrument is automatically set to a base frequency
10 of about 4 Hz, and an inflammation limiting effect is obtained at a frequency of about 6 Hz.

The instrument can also be used to obtain for instance beneficial effects in cases of tendinitis or acute inflammations. Then, the instrument is automatically set to a pain
15 relieving frequency about 4 Hz. In this case, the inflammation limiting frequency is also about 4 Hz.

For the above-mentioned frequency settings, a margin of error of about 10 % is
20 admissible.

The system in accordance with the invention can be used to influence any biological cellular structures and to realise a wide range of therapeutic or other beneficial effects. The term influencing/to influence must be interpreted in its most broad
25 significance, in which both temporary and permanent effects, phenomena or modifications in the biological cellular structure must be considered 'an influence'.

Within the framework of this invention, the instrument in accordance with this invention can be realised in many configurations that strongly differ from each other, according to, for instance, the envisaged field of application or the desired effect.
30

CLAIMS

- 5 1. A system for influencing of a biological cellular structure that makes use of a combination of light energy and magnetic energy, **characterised in that** this system comprises,
- At least one light source (2), (8),
 - a magnetic energy source (11) and
 - 10 - devices to adjust and/or modulate the frequencies and/or the phases and/or the amplitudes of the light and the magnetic field so that resonances and/or interferences can be obtained in the biological cellular structure.
- 15 2. A system for influencing of a biological cellular structure, in accordance with claim 1, characterised in that this system comprises a first (2) and a second light source (8), and that the second light source (8) is capable of generating light that is essentially more coherent than the light of the first light source (2).
- 20 3. A system for influencing of a biological cellular structure, in accordance with claim 2 characterised in that said first light source (2) is a full-spectrum lamp.
4. A system for influencing of a biological cellular structure, in accordance with claim 2 or 3, characterised in that the system comprises devices to operate the light coming from the first (2) and the second light source (8) alternately and/or with a phase shift.
- 25 5. A system for influencing of a biological cellular structure, in accordance with one of the previous claims, characterised in that the system is capable of generating pulsing magnetic fields.
- 30

6. A system for influencing of a biological cellular structure, in accordance with one of the previous claims, characterised in that said devices are capable of having the frequencies and/or the phases and/or the amplitudes of the magnetic field pulses and/or the light source pulses vary in accordance with a predetermined pattern and/or within a predetermined range in order to obtain said resonances and/or interferences.
7. A system for influencing of a biological cellular structure, in accordance with one of the previous claims, characterised in that the system (7), (9) comprises devices to polarise the light coming from the first light source (2) and/or the light coming from the second light source (8).
8. A system for influencing of a biological cellular structure, in accordance with one of the previous claims, characterised in that the second light source (8) comprises one or several LED light sources that are capable of generating single-phase light.
9. A system for influencing of a biological cellular structure, in accordance with one of the previous claims, characterised in that it is capable of generating a therapeutic effect in a human or animal body.

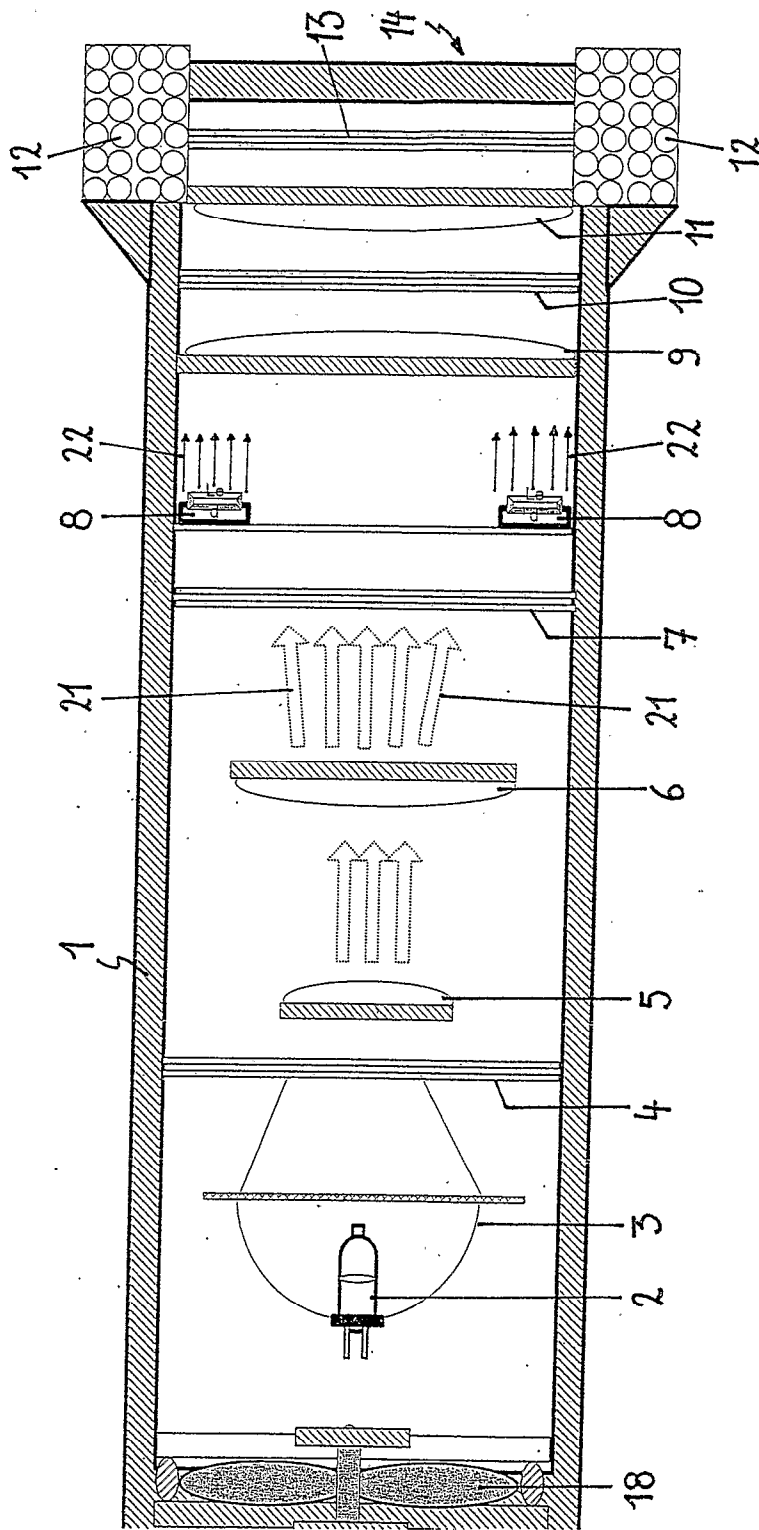


Fig. 1a

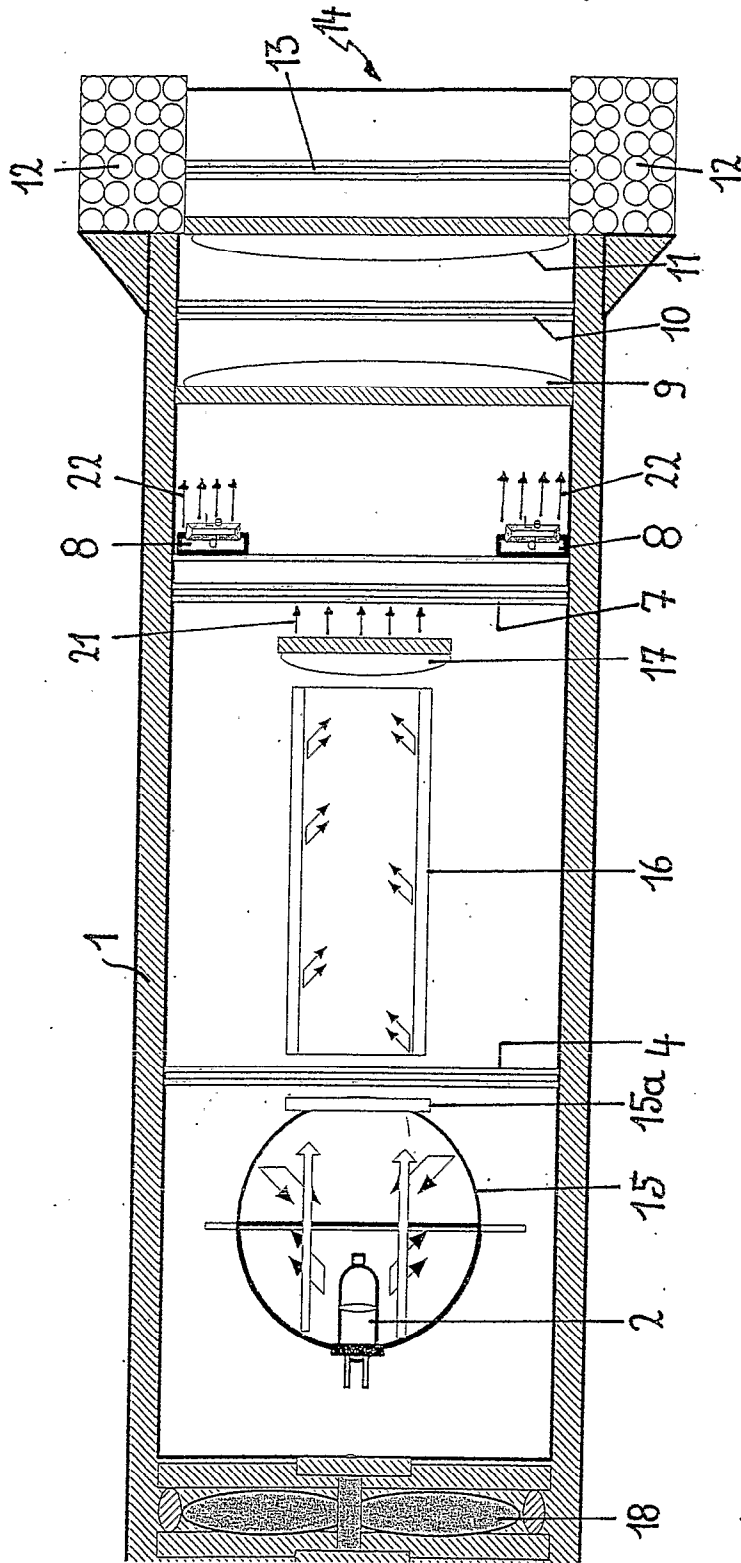


Fig. 1b

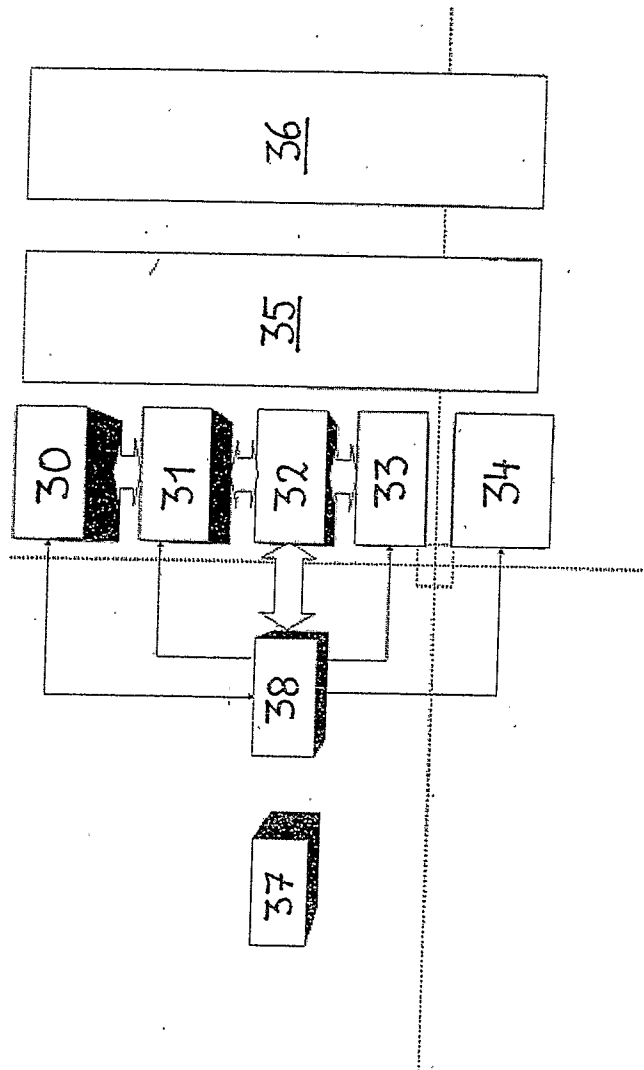


Fig. 3

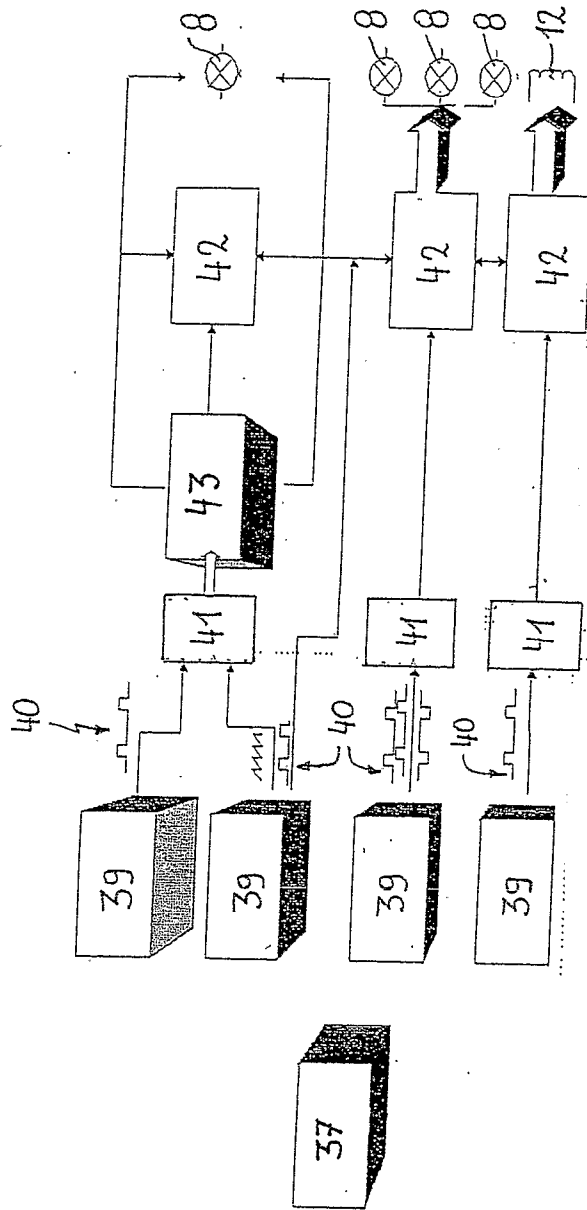


FIG. 4

INTERNATIONAL SEARCH REPORT

International Application No
PCT/EP2005/003304

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61N2/00 A61N5/06

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 7 A61N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	DE 31 01 715 A (MED TRONIK GMBH) 16 September 1982 (1982-09-16) cited in the application page 3, line 15 - page 5, line 11; figures -----	1-3,5-9
X	US 6 520 903 B1 (YAMASHIRO PATSY YUKIE) 18 February 2003 (2003-02-18) column 3, line 23 - column 4, line 44; figures -----	1,6,9
A	FR 2 639 834 A (TESSIER JEAN MICHEL ; DURAND MICHEL (FR)) 8 June 1990 (1990-06-08) cited in the application page 1, line 38 - page 3, line 5; figures ----- -/--	1,7

Further documents are listed in the continuation of box C.

Patent family members are listed in annex.

° Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *G* document member of the same patent family

Date of the actual completion of the international search

25 July 2005

Date of mailing of the international search report

03/08/2005

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Rakotondrajaona, C

INTERNATIONAL SEARCH REPORT

International Application No
PCT/EP2005/003304

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	<p>EP 0 228 537 A (ELEC SYSTEM VERTRIEBSGESELLSCH) 15 July 1987 (1987-07-15) cited in the application page 3, column 3, line 1 - column 4, line 6; figures</p> <p style="text-align: center;">-----</p>	1

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No PCT/EP2005/003304
--

Patent document cited in search report		Publication date		Patent family member(s)	Publication date
DE 3101715	A	16-09-1982	DE	3101715 A1	16-09-1982
US 6520903	B1	18-02-2003	NONE		
FR 2639834	A	08-06-1990	FR	2639834 A1	08-06-1990
EP 0228537	A	15-07-1987	DE	8532628 U1	17-04-1986
			CA	1301255 C	19-05-1992
			EP	0228537 A2	15-07-1987